

CAT IV 1kV Fused Test Leads

P/N 131350/R4

"Fused" Test Leads Provide Added Protection for User & Instrument!



Specifications

- Compatible with all Industry Standard 4mm Instrument Sockets
- Double Insulated, Bi-Color Silicone Cable boasts 250+ copper strands for maximum flexibility and overall performance
- Fused leads protect user from shock -even if the instrument is fused!
- Fuse is easily serviced without the use of tools



E112637

Complies with/Conforme avec
UL61010-1
CSA C22.2 No. 61010-1
With/Avec EN61010-2-31

***Rated 1000V CAT IV
Calibré 1000V CAT IV***

***Fuse Rating: 500mA/1000V/50kA
Calibre du fusible : 500mA/1000V/50kA***

SILVERTRONIC
LTD

Title: 1000V CAT IV RA Plug to
1000V CAT IV Fused Probe set

This drawing is not to be disclosed to a third
party without the written authority from the
company ©

Material: N/A

Rev
4
3
2
1
-

Details

First issue

Pre-Production issue

Date

17/05/07

17/05/07

Drawn

CS

CS

Part No:


131517

Project No: #####

1 Red & 1 Black 123365 Lead Assemblies

Fuse: 116048


OEM 1000V CAT IV Right Angle Plug: 125116

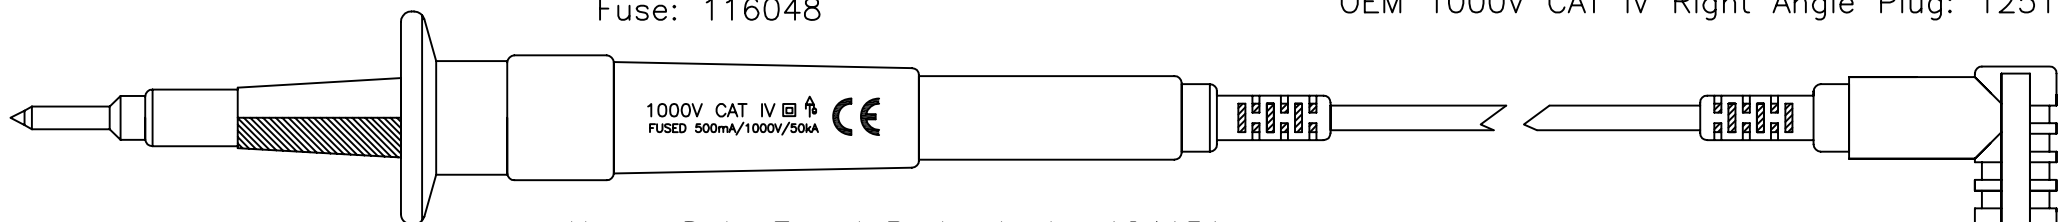

Fixed Tip Front: 124013

Heavy Duty Fused Probe body: 124151

Double Silicone Cable: 119054 cut 1250mm or 102523

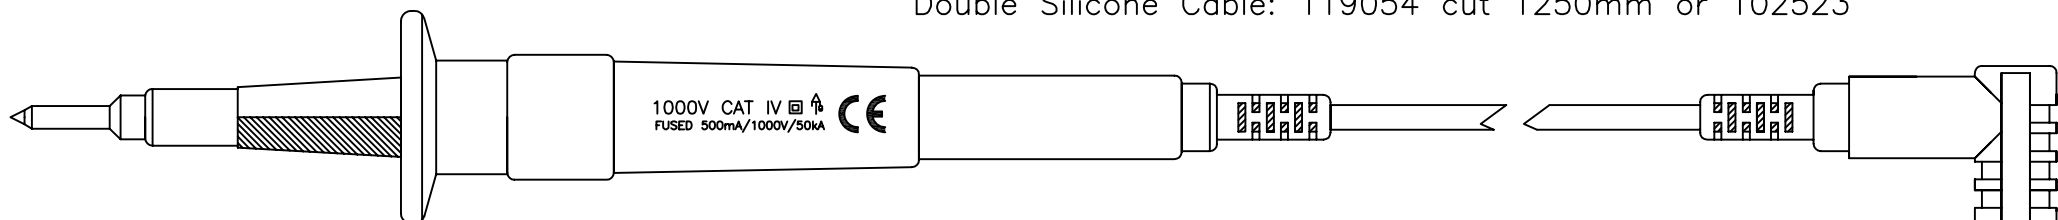

PRINTING ON REVERSE OF BODIES

Assembly Jig Numbers

#####=J###

#####=J###

#####=J###

#####=J###

Packaging: 119502 Wallet

Tolerances:
Cable Lengths +/- 5%

Do Not Scale All Dimensions In
MM

SILVERTRONIC

LEADS
...the way forward!

Leaside Industrial Estate,
Stockingswater Lane,
Enfield, Middx. EN3 7PH
Telephone: +44 (0)20 8805 3424
Facsimile: +44 (0)20 8805 3054

DECLARATION OF CONFORMITY

SILVERTRONIC Ltd. confirm that the products listed below have been Designed, Manufactured and Tested to, and therefore are fully compliant to;
IEC1010-1 1990 inc. Amendment 2-1995 & IEC1010-2-031 First Edition-1993
and thus meet **THE LOW VOLTAGE DIRECTIVE (LVD) 73/23/EEC and amending directive 93/68/EEC**

PRODUCT TYPE / DESCRIPTION				Heavy Duty CAT IV Fused Probe Leads	
PART No.				131350/R4	
IEC1010 RATING	VOLTAGE	1000	Volts	INSULATION CATEGORY	IV (4)

MAXIMUM RATED CURRENT	*0.5 as fuse	Amps
POLLUTION DEGREE	2	
INSULATION CATEGORY	DOUBLE/REINFORCED	

INCLUDES FOLLOWING ASSEMBLIES / COMPONENTS SUBJECT TO INDIVIDUAL TEST.	DESCRIPTION	PART No.
	Heavy duty fused body	124151
	CAT IV Right angle plug	125116
* Current limited to fuse fitted		



All Testing carried out by Third Party Testhouse
CRANAGE EMC TESTING Ltd.
(LVD TESTING DEPARTMENT)



www.silvertronic.com
e-mail: sales@silvertronic.com

Registration No. 1993292

North American Office
620 E. Smith Rd, Unit W-19
Medina, Ohio, 44256.
Toll Free: (866) 556 3308
Facsimile: (330) 722 2281